
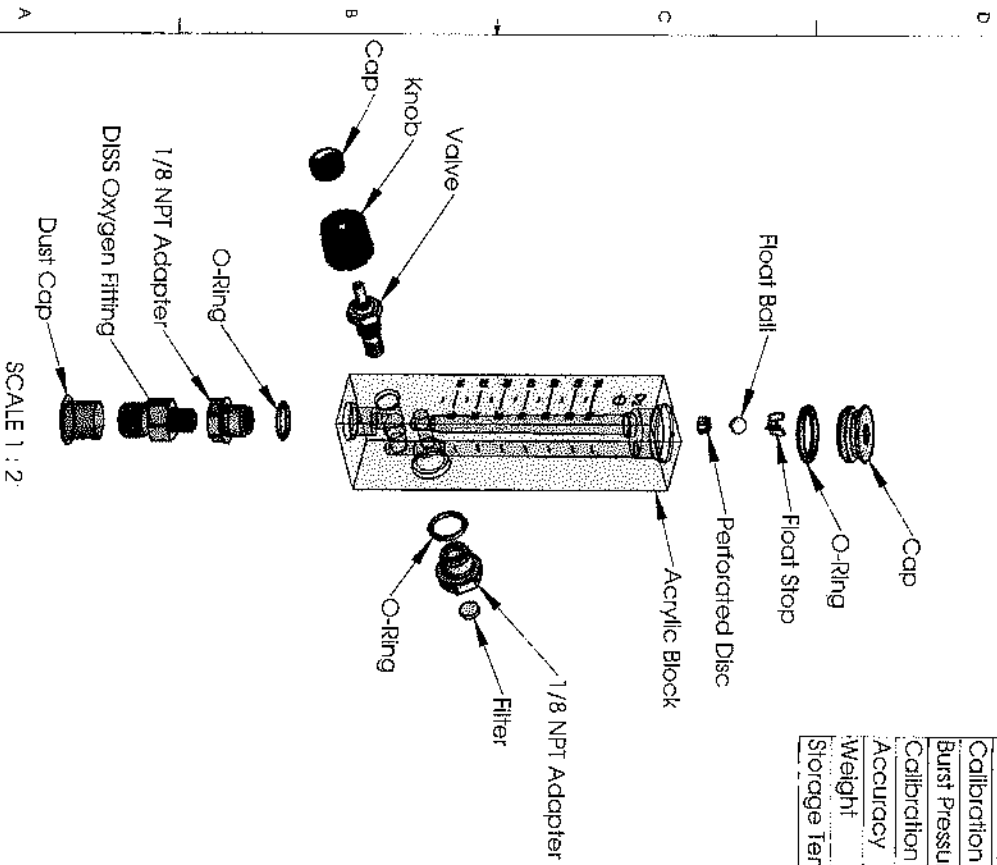
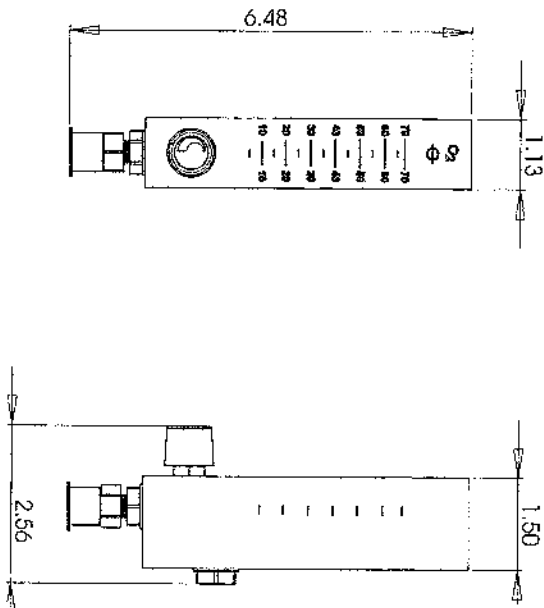


Flowmeter Performance Specifications	
Flow Range	0-70 LPM
Gas Type	Oxygen
Increments	5 LPM (starts at 5 LPM)
Calibration Pressure	50 psi
Burst Pressure	>150 psi
Calibration Temperature	70 °F (21 °C)
Accuracy	+/- 10% of indicated value
Weight	6.8 oz
Storage Temperature	-40 °F (-40 °C) to 140 °F (60 °C)



REVISIONS	
REV	DCOS AFFECTING THIS DRAWING
DATE	4/29/2010
INITIAL	REL. DCO # 5260
DATE	2/11/10
INITIAL	D. LARSEN

maxtec®
SALT LAKE CITY, UT

**SPECIFICATION,
0-70 LPM Flowmeter**

DESIGNED BY	E. LAVERY	2/9/15	CHECKED BY	D. LARSEN	2/11/15
DATE	2/9/15	DATE	2/11/15	DATE	2/9/15
DESIGNED BY	M. VILLARREAL	2/9/15	CHECKED BY	A. NEWTON	2/9/15
DATE	2/9/15	DATE	2/9/15	DATE	2/9/15




UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
AND PER ANSI Y14.5-1992

XX ±.01
XXX ±.005
XXXX ±.002

ORIGINATOR: A. NEWTON
SIZE: B
DWG. NO.: R220P40
SCALE: 1:2
SHEET 1 OF 1

8 7 6 5 4 3 2 1

Flowmeter Performance Specifications	
Flow Range	0-120 LPM
Gas Type	Oxygen
Increments	20 LPM (starts at 120 LPM)
Calibration Pressure	50 psi
Burst Pressure	>150 psi
Calibration Temperature	70°F (21°C)
Accuracy	+/- 10% of indicated value
Weight	6.8 oz
Storage Temperature	-40°F (-40°C) to 140°F (60°C)

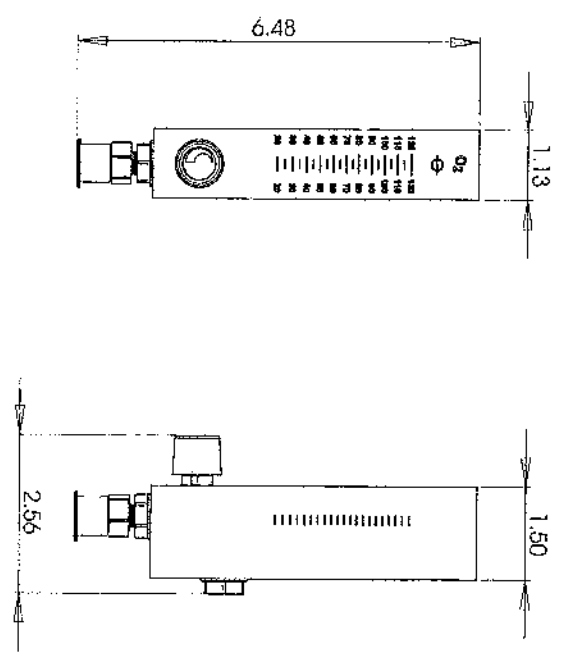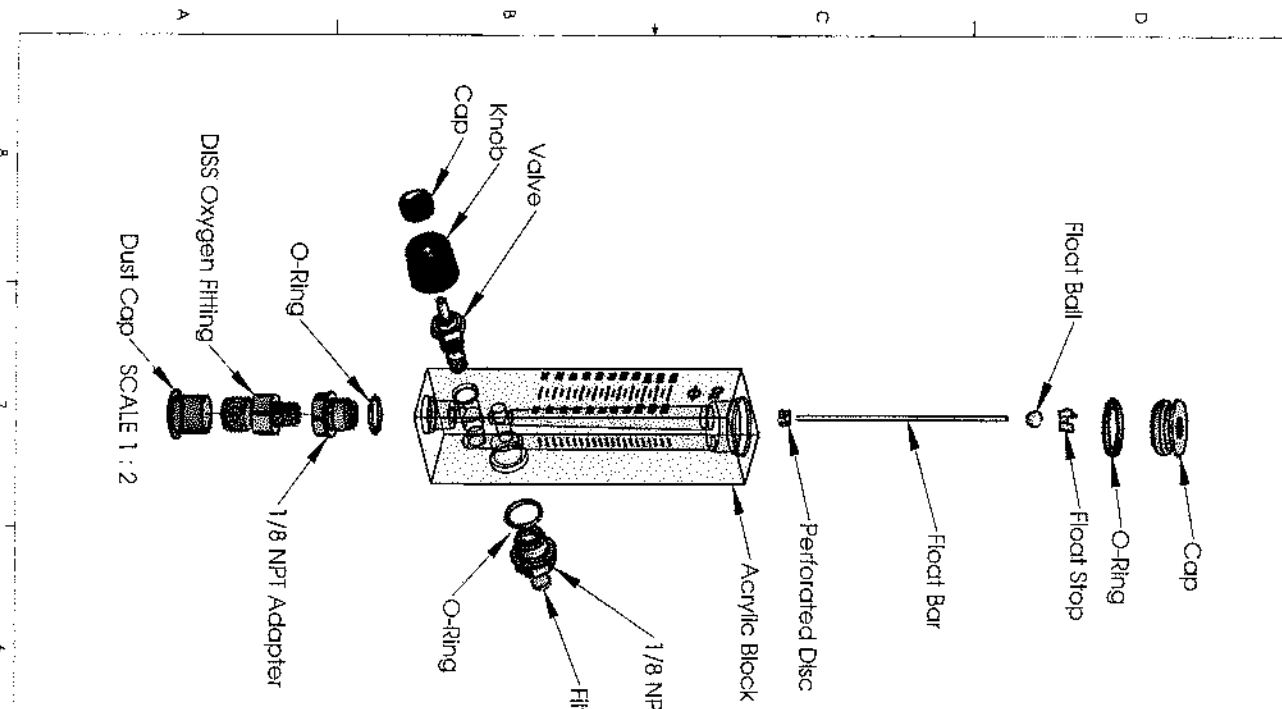





REVISIONS	
REV/DCOS AFFECTING THIS DRAWING	DATE
A INITIAL REL. DCO # 5260	2/11/15
	APPROVED
	D. LARSEN

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND PER ANSI Y14.5-1992			
ORGANIZATION	ANGLES	DATE	REV.
A. NEWTON	11°	2/6/15	A
DESIGNED	DATE	SIZE	DWG. NO.
D. LARSEN	2/11/15	B	R220P41
DRW	DATE	SCALE	1:2
A. NEWTON	2/9/15		
1 LAYER	2/9/15		
M. VALARRE	2/9/15		
See COP-2001 for details			

maxtec®
 SPECIFICATION,
 0-120 LPM Flowmeter

REVISIONS		DATE	APPROVER
REV: DCCS AFFECTING THIS DRAWING			
A INITIAL REL. DCO # 5260		2/11/15	D. LARSEN

Flowmeter Performance Specifications	
Flow Range	0-30 LPM
Gas Type	Oxygen
Increments	1 LPM (starts at 1 LPM)
Calibration Pressure	50 psi
Burst Pressure	> 150 psi
Calibration Temperature	70 °F (21 °C)
Accuracy	2-4: +/- .50 LPM, 5-30: +/- 10% of indicated value
Weight	6.8 oz
Storage Temperature	-40 °F (-40 °C) to 140 °F (60 °C)

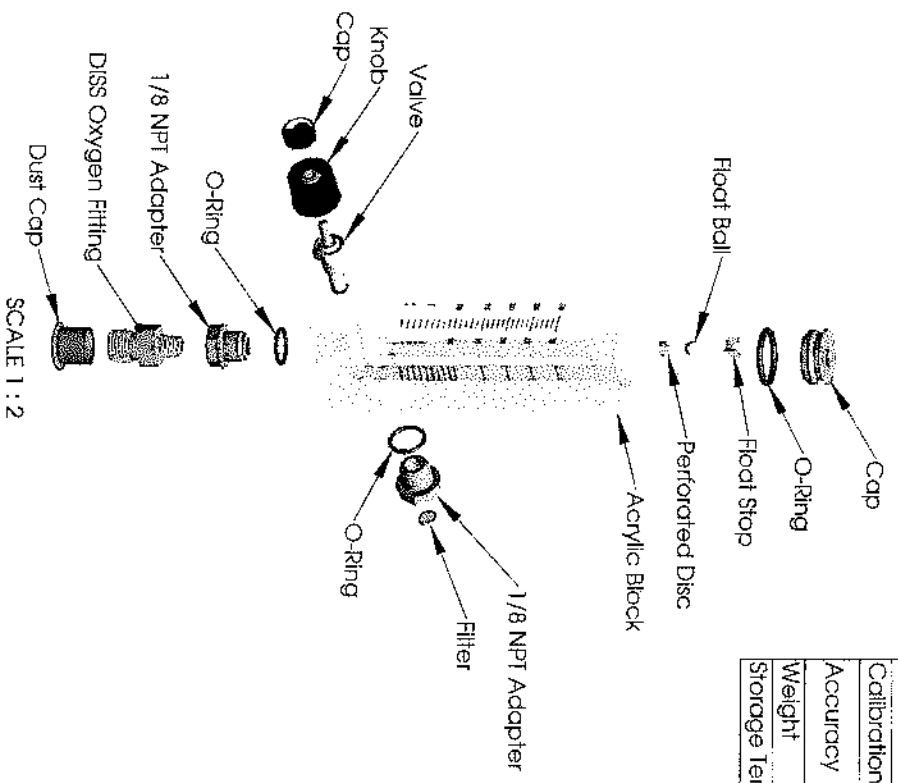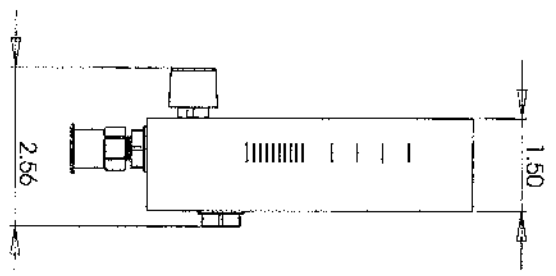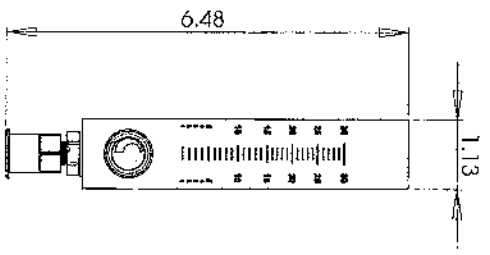

DATE	BY	DESCRIPTION
2/9/15	M. VILLARUEL	1st LAYER
2/9/15	A. NEWTON	2nd LAYER

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND PER ANSI Y14.5-1982	
XX ±.05	ANGLES
XXX ±.02	FLATS
ORGANATOR	A. NEWTON
DRAWN	D. LARSEN
DATE	2/11/15
SCALE: 1:2	
SHEET 1 OF 1	

maxtec®
SALT LAKE CITY, UTAH

**SPECIFICATION,
0-30 LPM Flowmeter**

SIZE DWG. NO. **R220P42**